

ANALIZA BIAŁEK



100015821

Laboratory of Analysis

Client: Lab Grade
Order number: 100015821
Name: BACTERIOSTATIC MIXING WATER
Number of samples: 1 vial

Batch number: LG-28537865-BW10
Recive date: 2026-07-01
Start date: 2026-07-10
End date: 2026-07-14

Sample identification

Substance	Method of taking a sample	Form
Benzyl Alcohol	Sample provided by customer	Transparent liquid in a glass vial


Results

Substance	Sample name	Content	Purity
Benzyl Alcohol	BACTERIOSTATIC MIXING WATER	0,97%	-----

Research comment

The test sample was applied in the amount of 3 μ l to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H₂O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peak of the sought substance appeared. Its content, when compared to the reference chromatogram, is 0,97%. Height the measurement error is + - 0,01%. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample

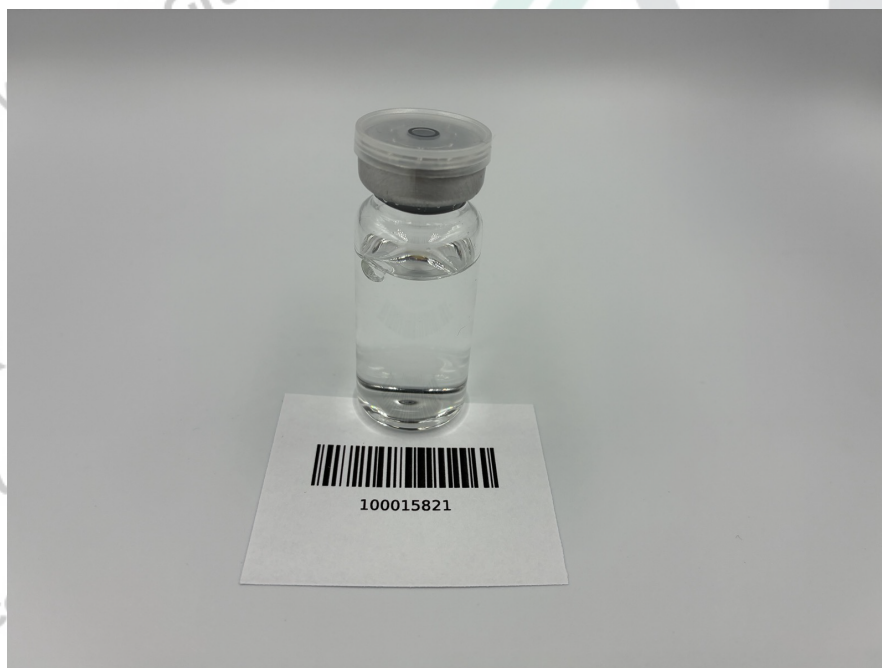


Password

5K92WT1C

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajęc




ANALIZA BIAŁEK



100015821

Chromatogram

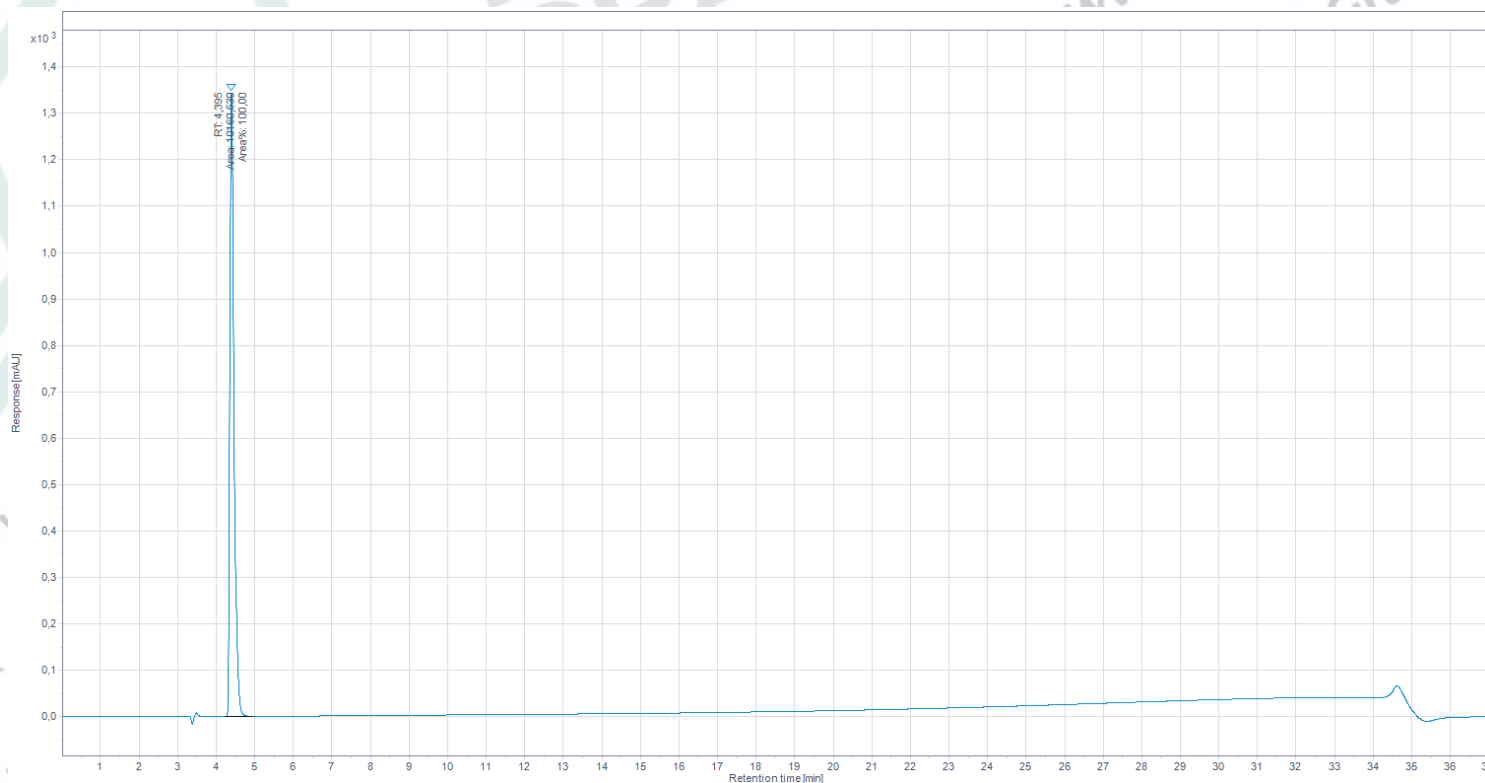

Method

Time	H2O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
27min	5%	95%
30min	5%	95%

Password

5K92WT1C

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław

Budynek DELTA

Lab technician:

Analysis and research specialist

mgr Arkadiusz Zajac