

ANALIZA BIAŁEK



100015799

Laboratory of Analysis

Client: Lab Grade
Order number: 100015799
Name: LAB GRADE CJC-1295 NO DAC
Number of samples: 1 vial

Batch number: LG-20056238-CJCND10
Receive date: 2026-07-01
Start date: 2026-07-10
End date: 2026-07-14

Sample identification

Substance	Method of taking a sample	Form
CJC-1295	Sample provided by customer	White powder in a glass vial


Results

Substance	Sample name	Content	Purity
CJC-1295	LAB GRADE CJC-1295 NO DAC 10MG	11,16mg	99%

Research comment

The test sample was applied in the amount of 3 μ l to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H₂O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peak of the sought substance appeared. Its content, when compared to the reference chromatogram, is 11,16mg. Height the measurement error is + - 0,05mg. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample

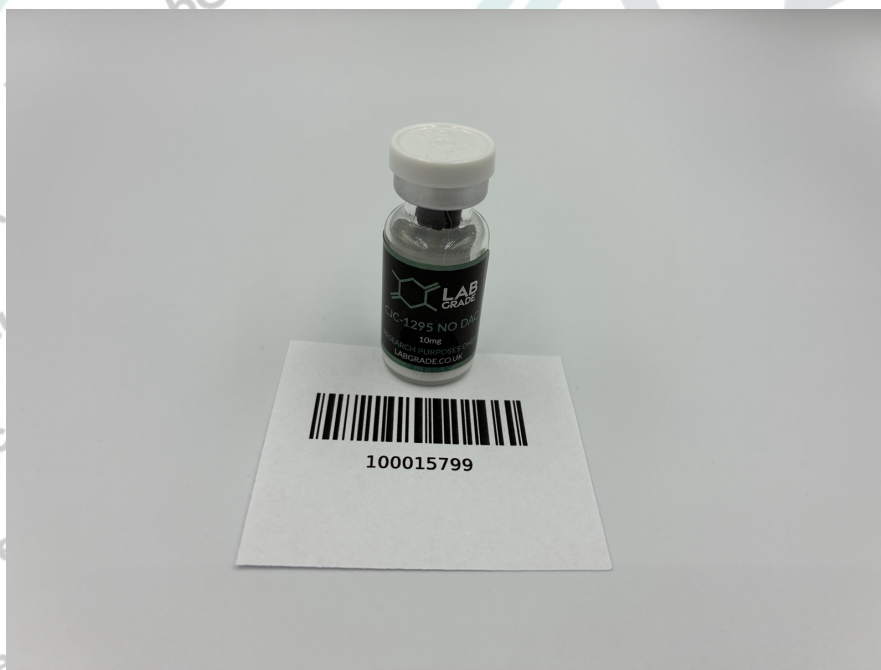


Password

F3S21K9L

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajęc




ANALIZA BIAŁEK



100015799

Chromatogram

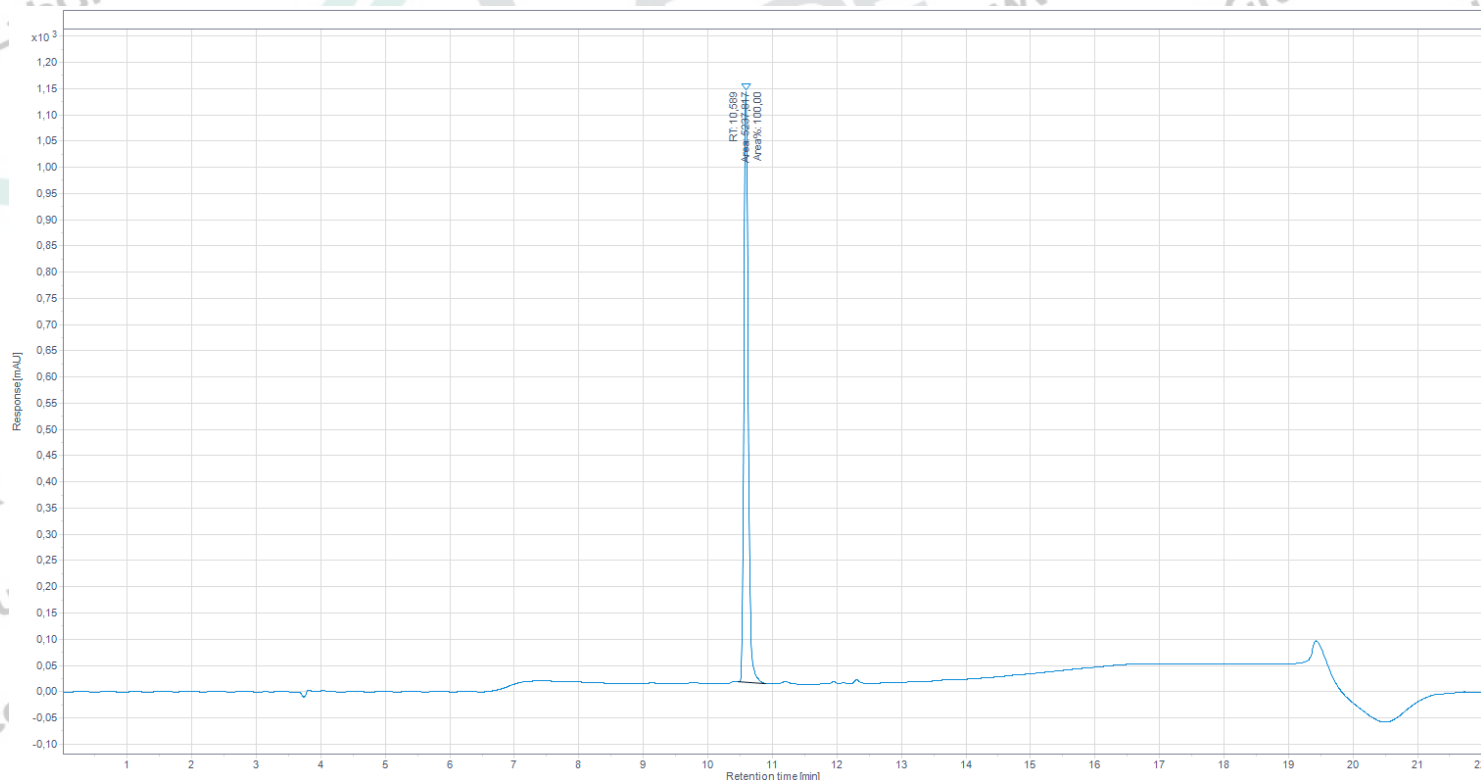

Method

Time	H2O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
12min	5%	95%
15min	5%	95%

Password

F3S21K9L

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:

Analysis and research specialist
mgr Arkadiusz Zajac